



ADLINK
TECHNOLOGY INC.

PXES-2301

6-slot PXI Express Chassis

User's Manual



Manual Rev.: PRELIMINARY

Revision Date: Sept. 9, 2016

Part No: N/A

Advance Technologies; Automate the World.

Revision History

Revision	Release Date	Description of Change(s)
PRELIMINARY	Sept. 9, 2016	Preliminary



NOTE:

Please note that this is a PRELIMINARY version of the User's Manual. While every effort has been made to ensure the contents hereof are currently accurate, subsequent releases may contain changes to the specification and operations, both minor and major, as well as entirely new chapters and modules not represented here.

For more information or if you have any questions, please visit our website at <http://www.adlinktech.com> or contact your local Sales Center, as detailed in Getting Service.

Preface

Copyright 2016 ADLINK Technology, Inc.

This document contains proprietary information protected by copyright. All rights are reserved. No part of this manual may be reproduced by any mechanical, electronic, or other means in any form without prior written permission of the manufacturer.

Disclaimer

The information in this document is subject to change without prior notice in order to improve reliability, design, and function and does not represent a commitment on the part of the manufacturer.

In no event will the manufacturer be liable for direct, indirect, special, incidental, or consequential damages arising out of the use or inability to use the product or documentation, even if advised of the possibility of such damages.

Environmental Responsibility

ADLINK is committed to fulfill its social responsibility to global environmental preservation through compliance with the European Union's Restriction of Hazardous Substances (RoHS) directive and Waste Electrical and Electronic Equipment (WEEE) directive. Environmental protection is a top priority for ADLINK. We have enforced measures to ensure that our products, manufacturing processes, components, and raw materials have as little impact on the environment as possible. When products are at their end of life, our customers are encouraged to dispose of them in accordance with the product disposal and/or recovery programs prescribed by their nation or company.

Trademarks

Product names mentioned herein are used for identification purposes only and may be trademarks and/or registered trademarks of their respective companies.

Conventions

Take note of the following conventions used throughout this manual to make sure that users perform certain tasks and instructions properly.



NOTE:

Additional information, aids, and tips that help users perform tasks.



CAUTION:

Information to prevent **minor** physical injury, component damage, data loss, and/or program corruption when trying to complete a task.



WARNING:

Information to prevent **serious** physical injury, component damage, data loss, and/or program corruption when trying to complete a specific task.

Table of Contents

Preface iii

List of Figures vii

List of Tables ix

1 Introduction 1

1.1 Features..... 1

1.2 Specifications..... 1

1.3 Schematics 5

1.4 Connectors, I/O, and Controls 10

1.4.1 Front & Rear Panels 10

1.4.2 Backplane..... 12

2 Getting Started 17

2.1 Package Contents 17

2.2 Cooling Considerations..... 18

2.3 Hardware Installation 22

2.3.1 Installing the System Controller 22

2.3.2 Installing Peripheral Modules 26

2.4 Rack Mounting..... 29

2.4.1 Powering Up the System 31

3 Monitoring the System..... 33

3.1 Installing the Monitor Utility..... 33

3.2 Monitoring the PXES-2301 33

3.2.1 Connect Control..... 34

3.2.2 Chassis Control and Alarm Threshold Setting..... 36

3.2.3 Chassis Status..... 38

A Appendix: Troubleshooting and Maintenance 41

A.1	Installation Problems.....	41
A.2	Basic Troubleshooting	42
A.3	Maintenance	42
A.3.1	Handling the Chassis.....	42
A.3.2	Cleaning the Exterior	43
A.3.3	Power Requirements	43
A	Appendix: Cooling Fan Replacement	45
	Important Safety Instructions.....	49
	Getting Service	53

List of Figures

Figure 1-1: Front View..... 5

Figure 1-2: Left Side View..... 6

Figure 1-3: Right Side View 6

Figure 1-4: Rear View 7

Figure 1-5: Top View..... 8

Figure 1-6: Underside View..... 9

Figure 1-7: PXES-2301 Front Panel 10

Figure 1-8: PXES-2301 Rear Panel..... 11

Figure 1-9: PXES-2301 PCIE Topology..... 12

Figure 1-10: PXES-2301 Backplane 13

Figure 1-11: Trigger Bus Bridge Capability..... 15

Figure 2-1: Cooling Clearances 21

Figure 2-2: Rack Mount Assembly..... 29

Figure 2-3: Right Side Bracket Mounting Holes 30

Figure 2-4: Left Side Bracket Mounting Holes 30

Figure 3-1: PXES-2301 Chassis Remote Mon. Utility..... 34

Figure 3-2: Log Options Dialog 35

Figure 3-3: Target Temperature Parameters 36

Figure 3-4: Chassis Temperature Sensors 38

This page intentionally left blank.

List of Tables

Table 1-1: PXITM-5 Low Power Chassis Specification..... 2

Table 1-2: PXES-2301 Low Power Chassis Specification..... 3

Table 1-3: PXITM-5 Normal Power Chassis Specification..... 3

Table 1-4: Front & Rear Panel Legend 11

Table 1-5: Front Panel LED Indicators..... 12

Table 3-1: Target Temperature Parameters Legend 37

This page intentionally left blank.

1 Introduction

The ADLINK PXES-2301 compact 6-slot PXI Express chassis, compliant with PXI Express and cPCI Express specifications, provides one system slot with three expansion slots and five hybrid peripheral slots, supporting a wide variety of enhanced-bandwidth testing and measurement applications. The hybrid-slot design accepts installation of Compact PCI, PXI, Compact PCI Express, and PXI Express modules in any peripheral slot for maximum flexibility. Built on a four-link PXI Express chassis with 8GB/s system bandwidth, the PXES-2301's peripheral slots are all connected with PCIe gen2 x4, with slot bandwidth up to 2GB/s.

The PXES-2301 implements ADLINK's ChassisWatch™ smart system monitoring control utility, reporting full chassis status including fan speed, system voltages, and internal temperature. Compact, rugged, half-rack size with efficient construction uniquely suits the PXES- 2301 for portable use with minimized space requirements. An industrial grade AC power supply delivers 320W performance under 50°C, with superior cooling capability. All in all, the PXES-2301 is an ideal PXI Express platform choice for practically any testing and measurement operation.

1.1 Features

- ▶ Compact construction with side carrying handle for portable application in a wide variety of testing environments
- ▶ Replaceable modular cooling fan reduces maintenance requirements
- ▶ High per-slot cooling capacity up to 38W
- ▶ ADLINK's ChassisWatch™ intelligent chassis management utility with automatic fan speed control and temperature/power status monitoring
- ▶ System bandwidth up to 8GB/S & peripheral bandwidth up to 2GB/s for all slots

1.2 Specifications

The PXES-2301 complies with the PXI™-5 Specification Rev.1.0 and accepts all modules compliant with the PXI™5, CompactPCI, and PICMG 2.0 specifications.

Power Supply

AC Input (*guaranteed by power supply design)	
Input voltage range	100 to 240 VAC
Operating voltage range*	90 to 264 VAC
Input voltage frequency	47 to 63 Hz
DC Output	
Maximum total usable power	320 W

Power Requirements

The PXI Systems Alliance provides normal power and low power chassis classifications, with the PXES-2301 power supply meeting the low power standard and providing interoperability between modules and chassis. Power rail specifications follow and are further detailed in the PXI™-5 PXI Express Hardware Specification, Section 4-11.

V	A	Total W
+5	+3.3	90
+3.3	9	
+12	6	
-12	0.5	
+5 AUX	1	

Table 1-1: PXI™-5 Low Power Chassis Specification

V	A	Total W
+5	20	320
+3.3	20	
+12	30	
-12	0.8	
5 AUX	3.5	

Table 1-2: PXES-2301 Low Power Chassis Specification

V	A	Total W
+5	19	290
+3.3	24	
+12	21	
-12	1.25	
5 AUX	1	

Table 1-3: PXI™-5 Normal Power Chassis Specification

10 MHz System Reference Clock (10 MHz REF)

Maximum clock skew between slots	300 ps
Built-in 10 MHz clock Accuracy	±25 ppm

100 MHz System Reference Clock: PXESe_CLK100

Maximum slot-to-slot skew	100 ps
Accuracy	±25 ppm

Cooling

Fans	2 sets of 100.2FM fans
Per-slot cooling capacity	38.2 W (verified by 50°C chamber test)

Physical

Slots	6 total, as follows: ▶ 1x system ▶ 5x hybrid peripheral
Dimensions	220.8mm (W) x 319.6mm (D), 177.8mm (H) (8.7 x 12.58 x 7 in.)
Weight	11.9 kg (26.2 lb)

Environmental

Storage	Ambient temperature: -20 to 70°C Relative humidity: 10 to 90%, noncondensing
Operating	Ambient temperature: 0 to 50°C Relative humidity 20 to 80%, noncondensing
Functional shock	30 G, half-sine, 11 ms pulse duration
Random Vibration	Operating: 5 to 500 Hz, 0.21 Grms, 3 axes Nonoperating: 5 to 500 Hz, 2.46 Grms, 3 axes
Sound Pressure Level (at operator position) Tested in accordance with ISO 7779	Auto fan (up to 25 °C ambient) 46.3 dBA High fan 64.5dBA
Sound Power	Auto fan (up to 25 °C ambient) 56.0 dBA High fan 76.0 dBA

Certification

Emissions Compliance	FCC/ICES-003 (USA / Canada): Class A - EN 61326-1 CE (Europe): Class A - EN 61326-1
Safety	CE/LVD (Europe, mandatory for devices with supply voltage exceeding 50VAC/ 75VDC): EN 61010-1

1.3 Schematics



NOTE:

All dimensions are shown in mm (millimeters)

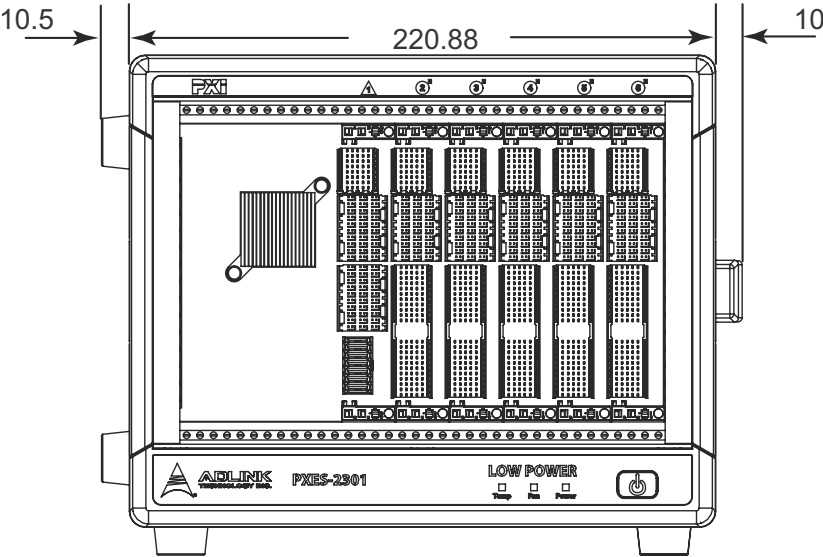


Figure 1-1: Front View

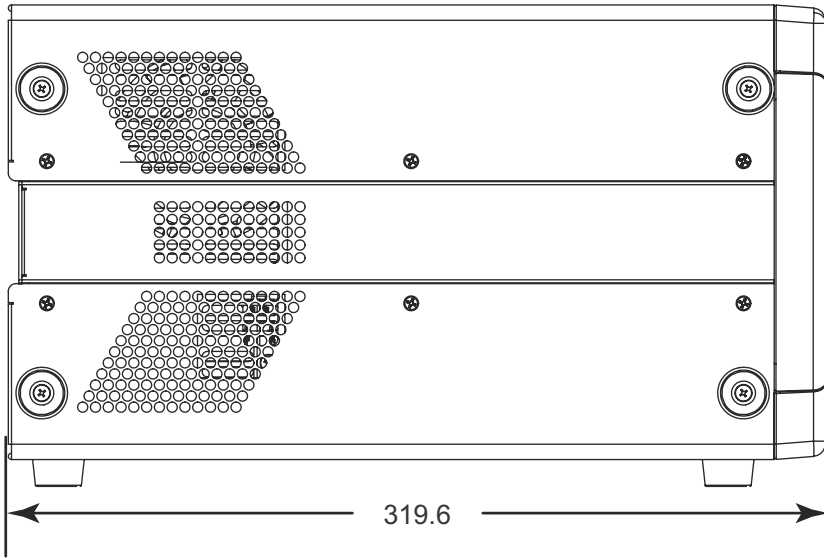


Figure 1-2: Left Side View

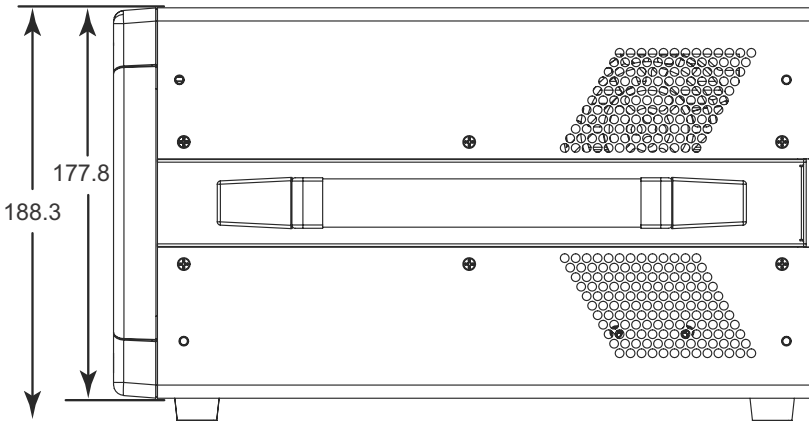


Figure 1-3: Right Side View

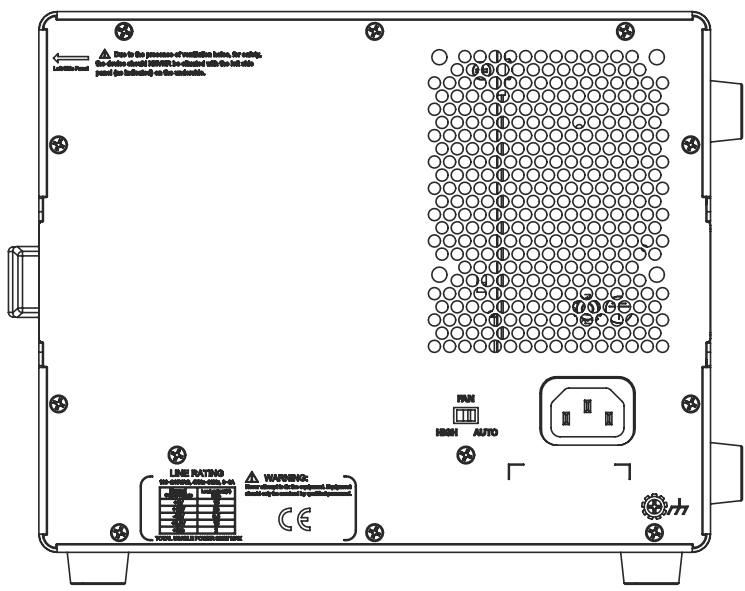


Figure 1-4: Rear View

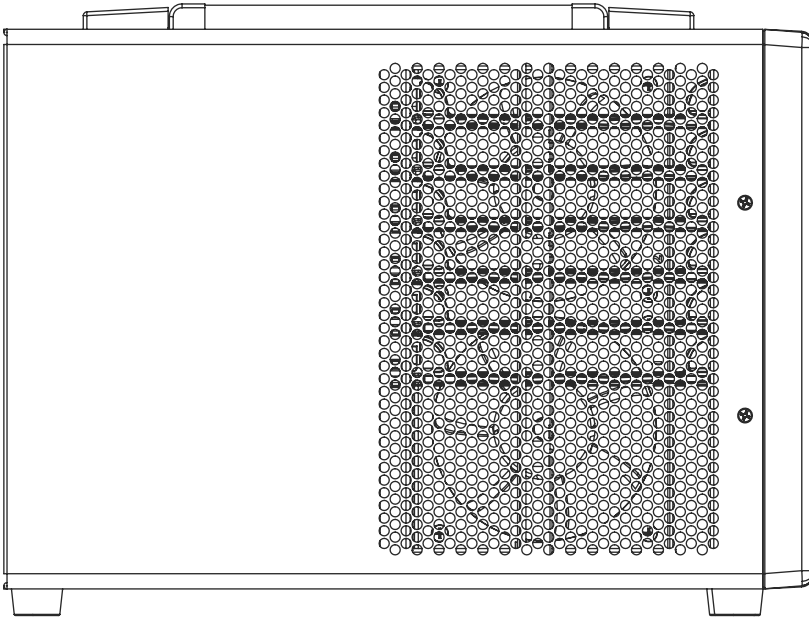


Figure 1-5: Top View

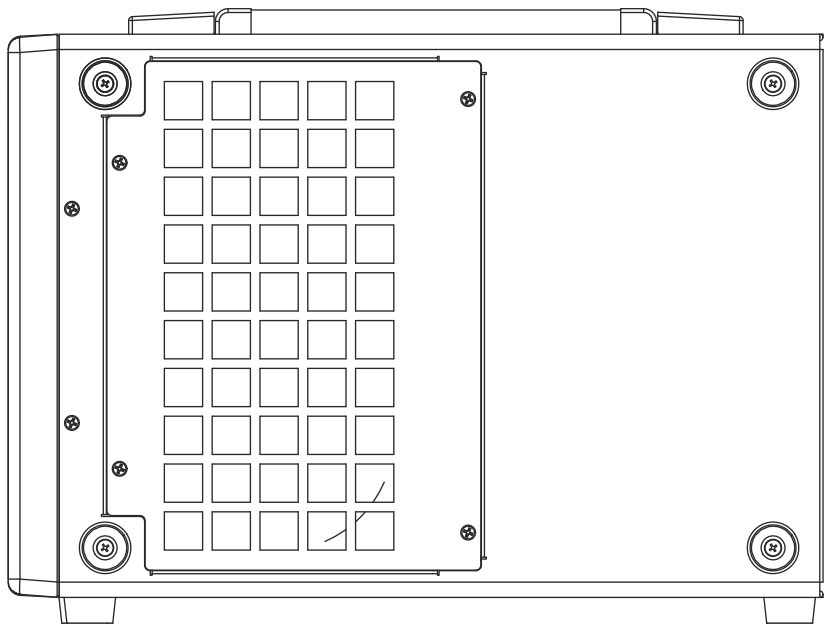


Figure 1-6: Underside View



Figure 1-8: PXES-2301 Rear Panel

	Feature	Details
A	Power	Powers the chassis on and off
B	Chassis Status LED	Temperature, Fan, and Power (L to R), functions (See “Front Panel LED Indicators” on page 12)
C	Fan Switch	In HIGH position, fans operate at maximum speed, in AUTO, fans run based on monitored chassis temperature
D	Universal Power	Accepts C13 power outlet-equipped connection
E	Chassis Ground Lug	For attachment to ground via ground lead

Table 1-4: Front & Rear Panel Legend

Status	Temperature (Amber)	Fan (Green)	Power (Blue)
On (Lit)	N/A	Fans operating normally	DC voltage supply is normal
Off	Temperature is normal	Chassis is powered down	Chassis is powered down
Blinking	One or more temperature sensors exceeds threshold temperature (default 70°C)	One or more fans falls below threshold speed (default is 800RPM)	One or more power rails exceeds threshold settings (defaults are $\pm 5\%$ for 5V, 3.3V, +12V, and -12V)

Table 1-5: Front Panel LED Indicators

1.4.2 Backplane

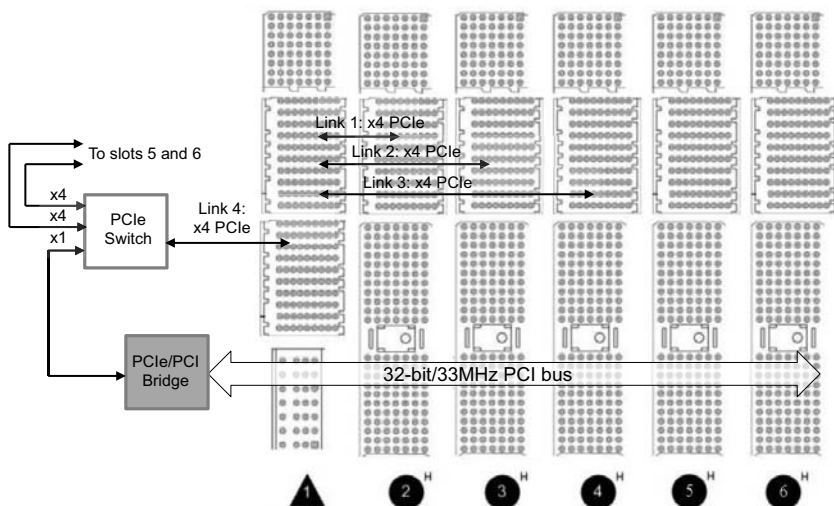


Figure 1-9: PXES-2301 PCIe Topology

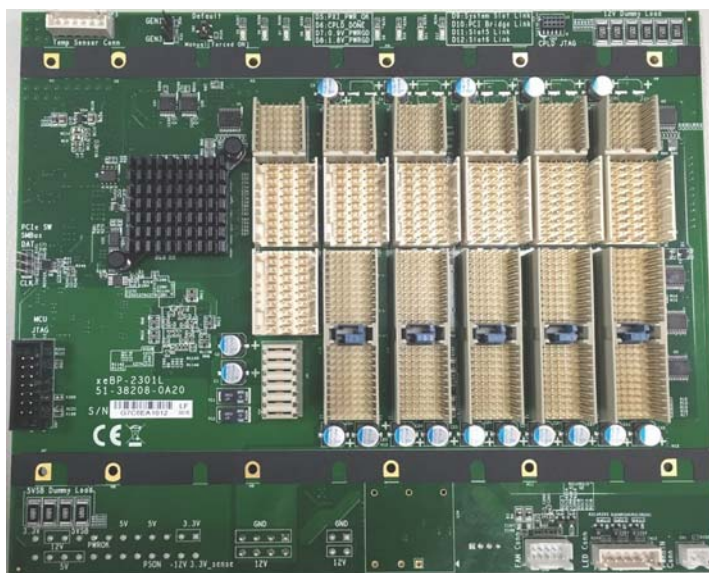


Figure 1-10: PXES-2301 Backplane



NOTE:

For details of chassis temperature detection, please see “Chassis Temperature” on page 38

PCI Express Link Capability

The PXES-2301 backplane follows a 4 link x 4 lane PCIe switch fabric configuration, as defined by Compact PCI Express and PXI Express specifications. The backplane routes three system slot x4 PCI Express links to 2nd to 4th peripheral slots directly. The fourth link is routed to a PCI Express switch, divided to x4 PCI Express links to 5th and 6th peripheral and x1 link to PCIe/PCI switch for 32-bit/33 MHz PCI bus to all hybrid slots.

The configuration delivers balanced PCI Express topology, with all peripheral slots sharing system bandwidth (x4) equally.



NOTE:

Connector pin assignments of the PXI Express System Controller Slot, PXI Express System Timing Slot, PXI Express Hybrid Peripheral Slots, and PXI Express Peripheral Slots comply with the default pin assignments as defined in PXITM5 PXI Express hardware specification Rev.1.0.

PXI Express System Controller Slot

The System Controller slot is Slot 1 of the chassis as defined by the PXI specification. The PXES-2301 chassis can accommodate a PXI Express system controller that occupies width up to 4 slots. As defined in the PXES specification, three controller expansion slots allow the controller to expand to the left to prevent the controller from using up peripheral slots.

PXI Express Hybrid Peripheral Slots

5 PXI Express hybrid peripheral slots are all connected with PCIe x4 lanes. Each can accommodate a 3U PXI Express/Compact PCI Express/hybrid slot compatible with PXI-1/Compact PCI peripheral modules. The hybrid peripheral slots provide PXI Express functionality (excluding DSTAR and PXI Star) and 32-bit PXI functionality.

Local Bus

The local bus on a PXI backplane is a daisy-chained bus that connects each peripheral slot with adjacent peripheral slots to the left and right. The quantity of local bus lines is decreased from thirteen to one on a PXI Express backplane. The remaining local bus line can transmit analog or digital signals between modules.

Trigger Bus

All six PXES-2301 slots share eight trigger lines, through which PXI and PXI Express modules can exchange trigger or clock signals via the trigger bus, allowing precisely timed response to asynchronous external events the system is monitoring or controlling.

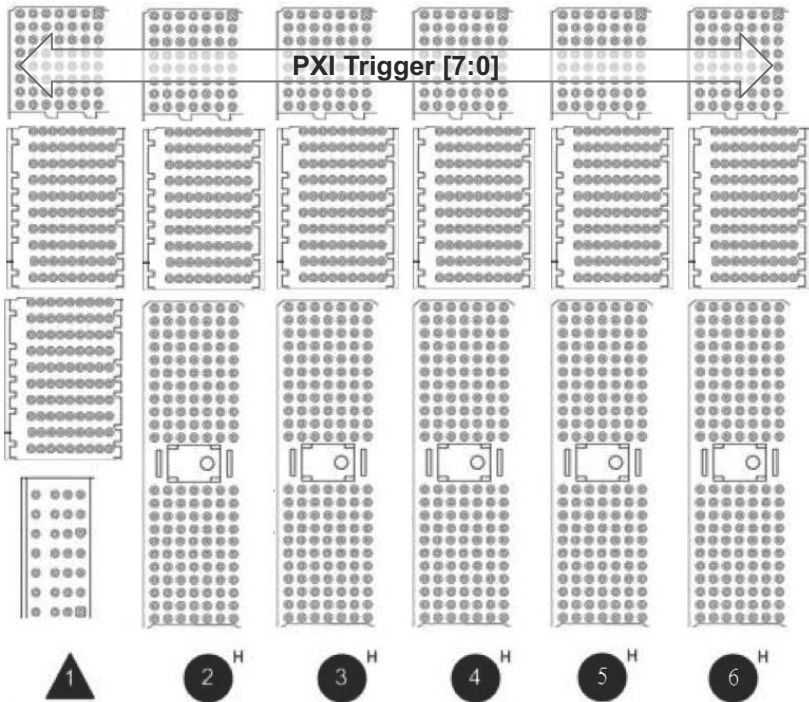


Figure 1-11: Trigger Bus Bridge Capability

Reference Clock

The PXES-2301 backplane supplies a single-ended 10MHz reference clock (PXI_CLK10) and differential 100MHz clock (PXIe_CLK100) to each peripheral slot for inter-module synchronization. The independent buffers drive the clock signal to each peripheral slot.

These common reference clock signals can synchronize multiple modules in a PXI Express chassis. PXI modules with phase-lock loop circuits can lock reference clocks to generate an in-phase timebase.

This page intentionally left blank.

2 Getting Started

This chapter describes procedures for installing the PXES-2301 and making preparations for its operation. Please contact ADLINK or authorized dealer if there are any problems during the installation.



NOTE:

Diagrams and illustrated equipment are for reference only. Actual system configuration and specifications may vary.

2.1 Package Contents

Before unpacking, check the shipping carton for any damage. If the shipping carton and/or contents are damaged, inform your dealer immediately. Retain the shipping carton and packing materials for inspection. Obtain authorization from your dealer before returning any product to ADLINK.

Please ensure that the following items are included in the package.

- ▶ PXES-2301 Chassis
- ▶ Power cords
- ▶ Filler panel kit for unused/reserved slots including five 1-slot panels
- ▶ Quick Start Guide

If any of these items are missing or damaged, contact the dealer from whom you purchased the product. Save the shipping materials and carton in case you want to ship or store the product in the future.




WARNING:


Do not install or apply power to equipment that is damaged or missing components. Retain the shipping carton and packing materials for inspection. Please contact your ADLINK dealer/vendor immediately for assistance and obtain authorization before returning any product.

2.2 Cooling Considerations

Two 100.2FM fans on the underside of the PXES-2301 draw cool air through apertures on the bottom and over the PXI/PXIe modules, to be exhausted through the top of the chassis.

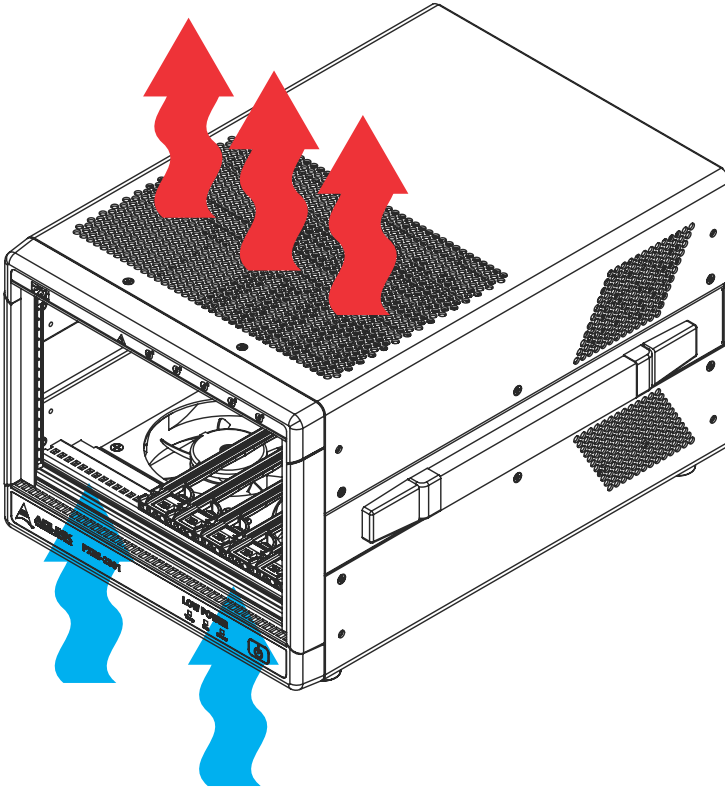

For power supply cooling, PSU fans draw cool air from the right side of chassis to be exhausted to the rear and left sides of the chassis

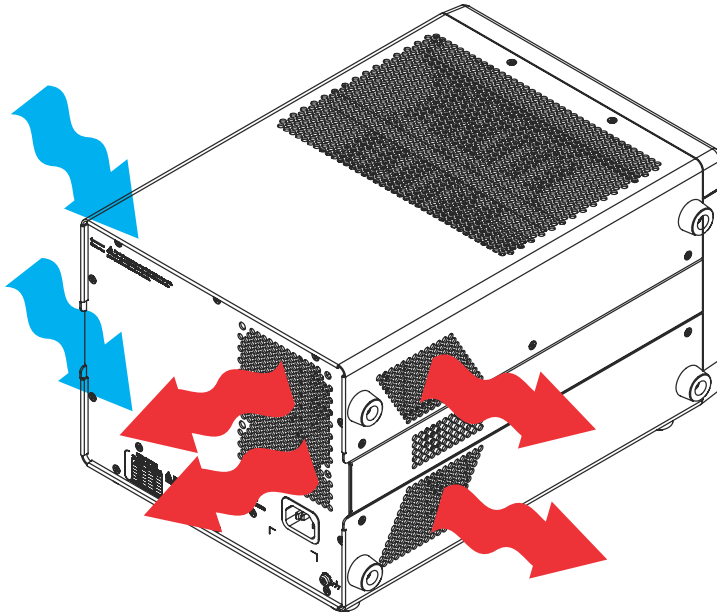

The PXES-2780 should be situated on a bench top or in an instrument rack, maintaining at least 1U (44.5 mm/1.75 in.) clearance from all ventilation apertures. Further, the 12.7mm/0.5 in. height of the rubber feet on the underside must be maintained to allow air intake.

The PXES-2301 smart fan control system detects the inner chassis temperature related to intake air temperature as the basis for fan speed control when in Auto Fan Speed. The user should be aware that the temperature in proximity to the chassis may exceed the ambient room temperature due to the presence of surrounding equipment and/or blockages, and may reach the upper operating temperature limit of 50°C when the environmental temperature may still be lower.

While the PXES-2301 supports bidirectional setup, chassis direction cannot be configured with the right side carrying handle on the bottom, which can impede cooling functions.



NOTE:

To sustain required air flow, always install provided filler panels in unused slots.



NOTE:

All dimensions are shown in mm (millimeters)

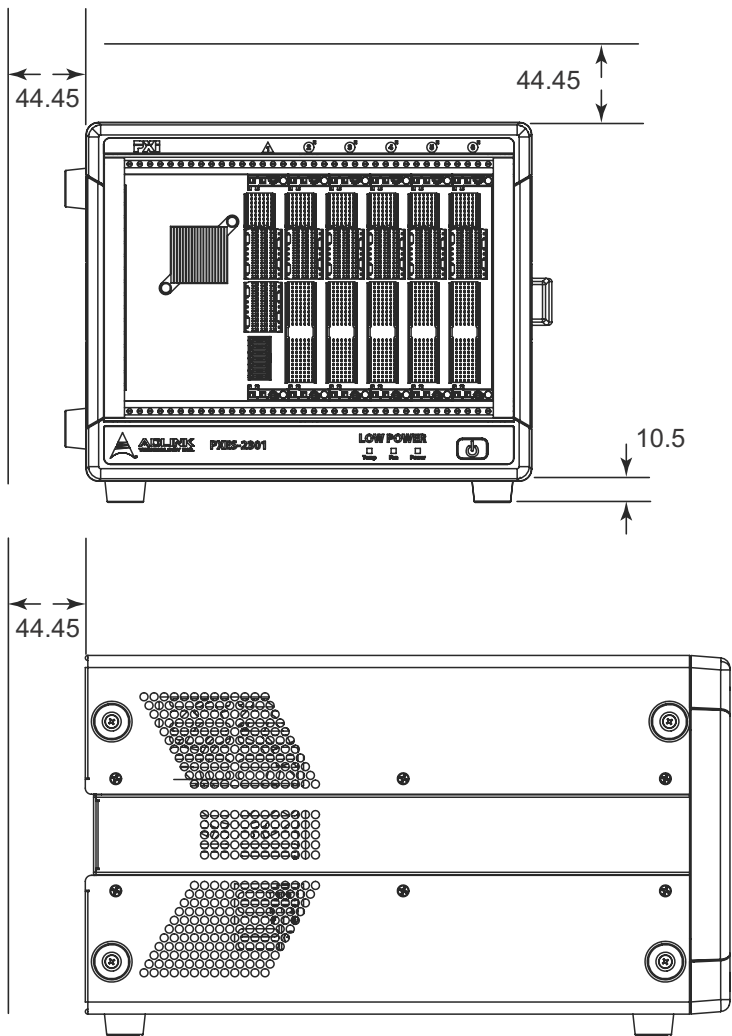


Figure 2-1: Cooling Clearances

2.3 Hardware Installation

2.3.1 Installing the System Controller

The PXES-2301 incorporates a system controller slot supporting a PXI Express system controller of up to 4 slot width.

1. Ensure the CPU, memory module(s), and storage device(s) are properly installed on the system controller
2. Locate the system controller slot (Slot 1).



3. Depress the system controller module's latch to release.




4. Align the module's top and bottom edges with the card guides, and carefully slide the module into the chassis.



5. Lift the latch until the module is securely seated in the chassis backplane


6. Fasten the screws on the module front panel, and connect all devices to the system controller.

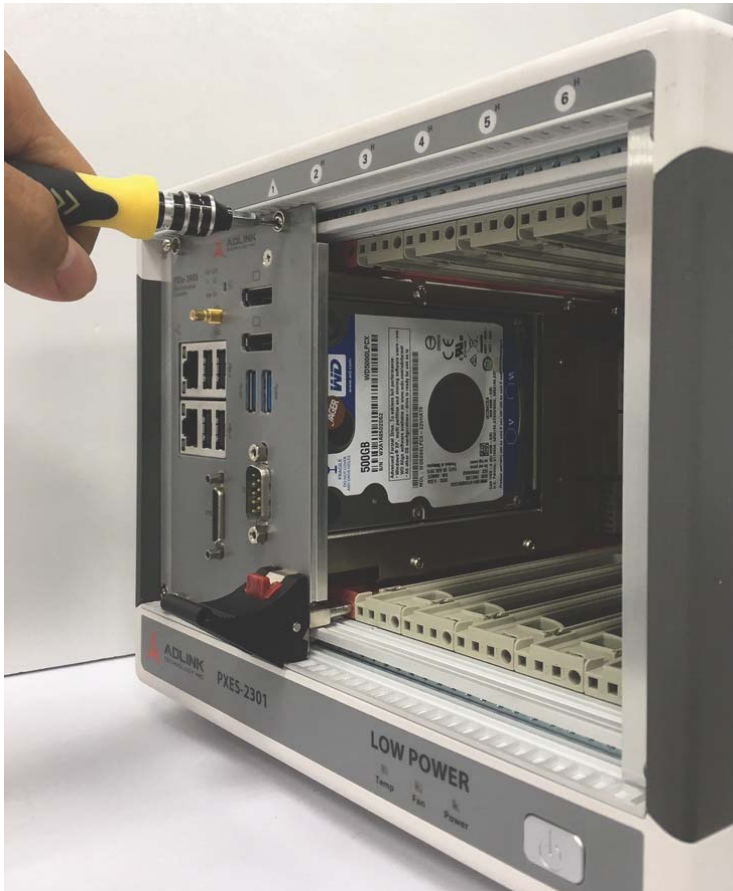


2.3.2 Installing Peripheral Modules

The PXE-2301 supports up to seventeen peripheral modules, including a system timing module.


1. Select an available peripheral slot (2 to 6)
2. Depress the peripheral module's latch and align the module's top and bottom edges with the card guides.
3. Carefully slide the module into the chassis.

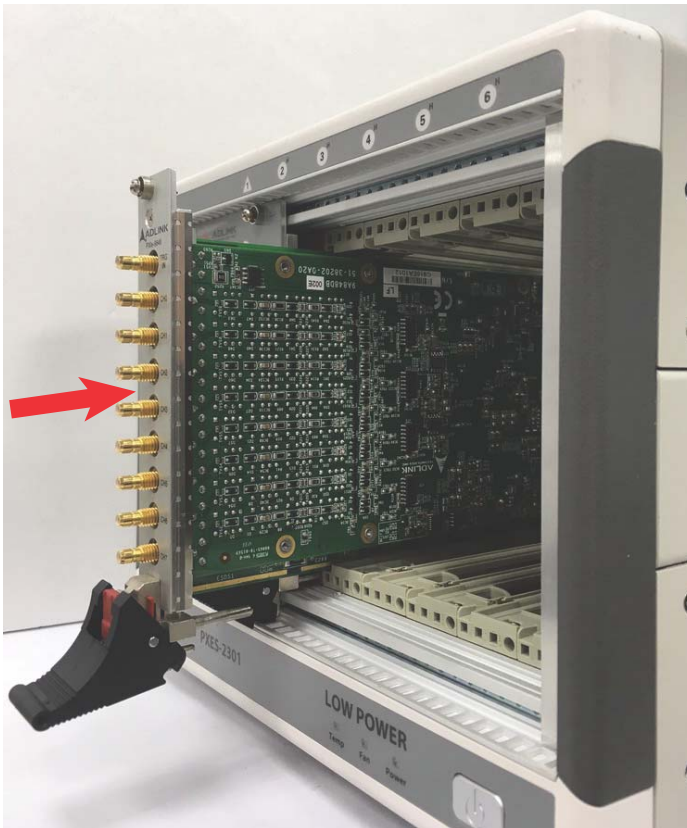

4. Lift the latch until the module is securely seated in the chassis backplane.

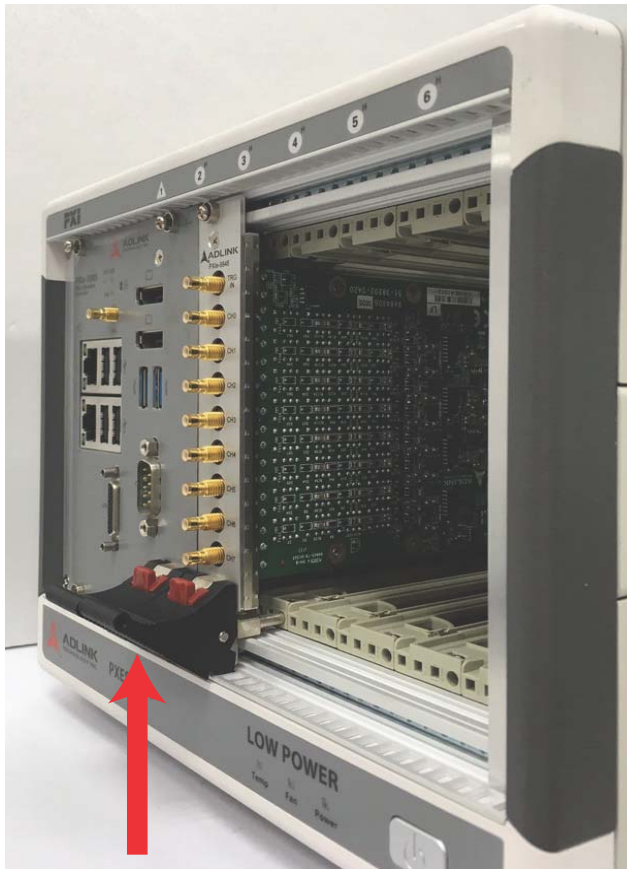

5. Fasten the screws on the module's front panel.

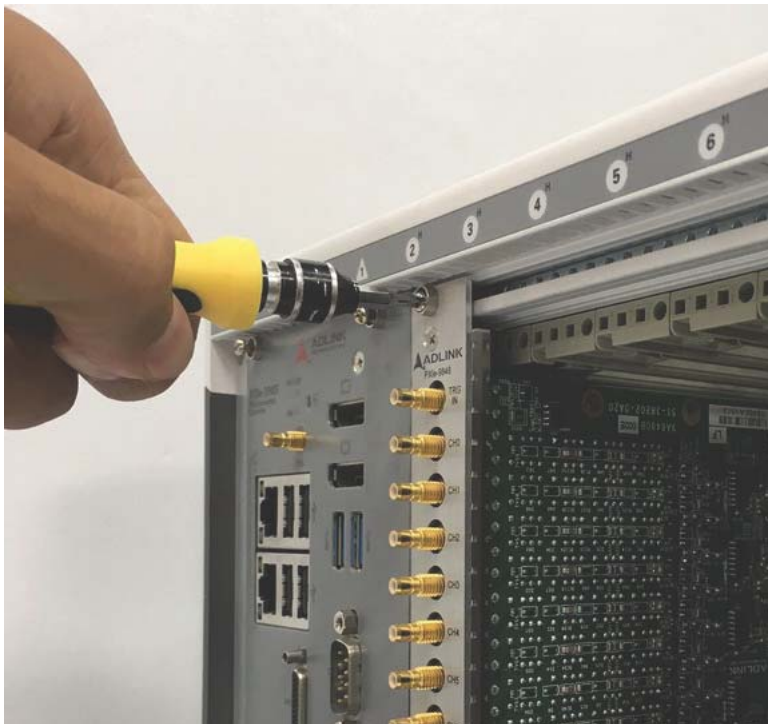

6. Repeat steps 1 to 5 to install additional PXI or PXES peripheral modules.



NOTE:

To improve efficiency of heat dissipation, after installing all PXES modules, please install filler plates for any unused slots.

2.4 Rack Mounting

ADLINK provides hardware for optional installation of the PXES-2301 to a rack. The kit (order name PXES-2301 Rack Mount Kit) flexibly recesses the PXES-2301 in the rack, accommodating external mechanical parts on the front side, such as cables and mass interconnect modules.

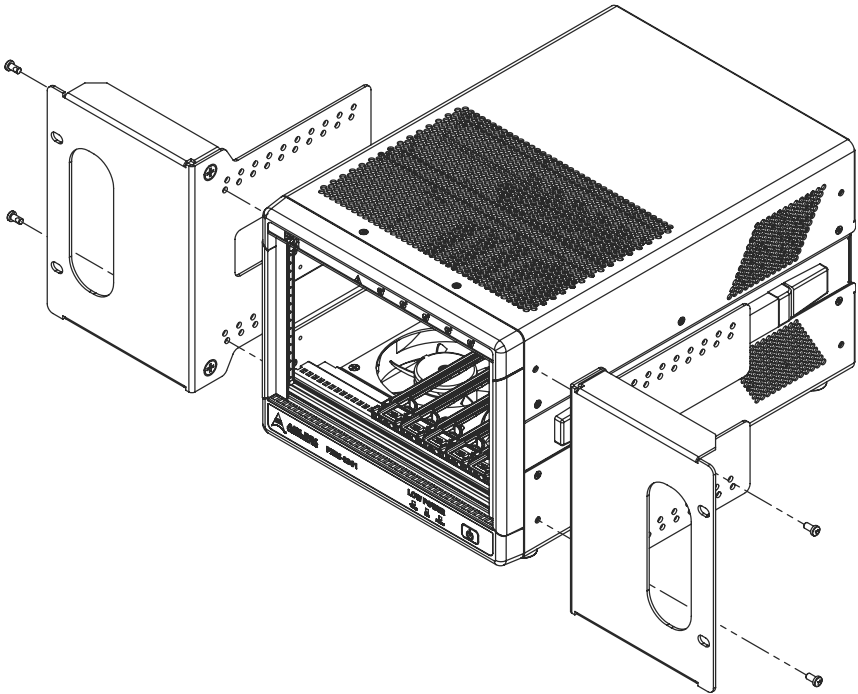


Figure 2-2: Rack Mount Assembly

For the right side bracket, place screws in the holes marked R.

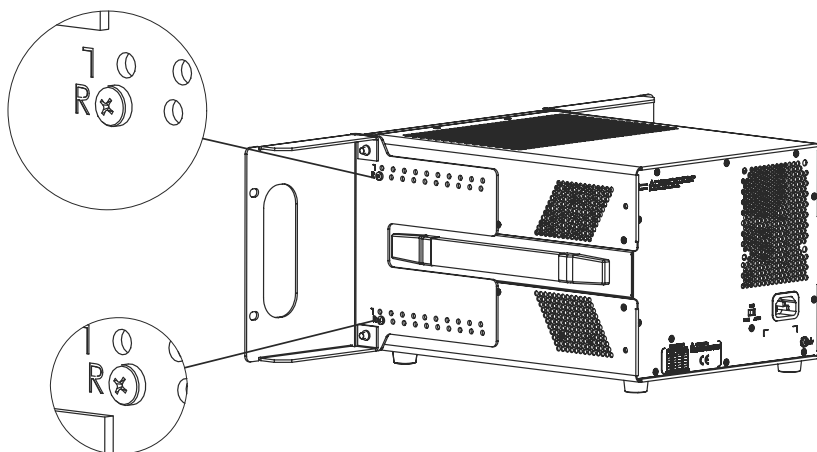


Figure 2-3: Right Side Bracket Mounting Holes

And for the left side bracket, use the holes marked L.

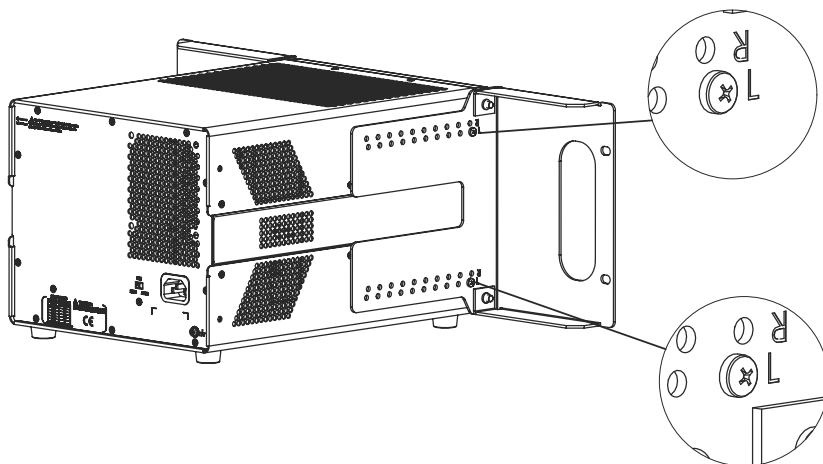


Figure 2-4: Left Side Bracket Mounting Holes

- 1.Remove carrying handle from the right side
- 2.Remove the four rubber feet from the left side

3. Install the mounting brackets on both sides of the chassis using the provided M4 screws. Position of the mounting brackets can be adjusted via a range of screw holes to recess the chassis in the rack by any distance
4. Install the chassis in the rack using eight screws (not included).

2.4.1 Powering Up the System

The PXES-2301 is equipped with a 100 VAC to 240 VAC universal power supply unit requiring no input voltage selection.

1. Connect one end of the supplied power cord to the power inlet located at the rear side of the chassis.
2. Plug the other end of the AC power cord to a properly grounded wall socket or power strip.
3. Press the power button. The Power LED (blue) lights up immediately
4. To power off the chassis, press the power button.

This page intentionally left blank.

3 Monitoring the System

The PXES-2301 chassis provides advanced system monitoring and control. Chassis conditions, including internal temperature, fan speed, and DC voltage can all be monitored on the system controller.

Communication with the chassis monitoring control unit is available using an embedded controller, such as ADLINK PXIe-3985/3975/3935, to access the SMBus located on the system slot (1st slot).

3.1 Installing the Monitor Utility

Download the ADLINK PXI platform service package including system monitoring utility from: <http://www.adlinktech.com>.

Double-click the **Setup.exe** file to begin installation.

3.2 Monitoring the PXES-2301

ADLINK provides the PXES-2301 Chassis Remote Mon. Utility to monitor the status of the PXES-2301.

As shown, the utility is divided into three interface categories: Connect Control, Remote Status & Control, and Chassis Status.

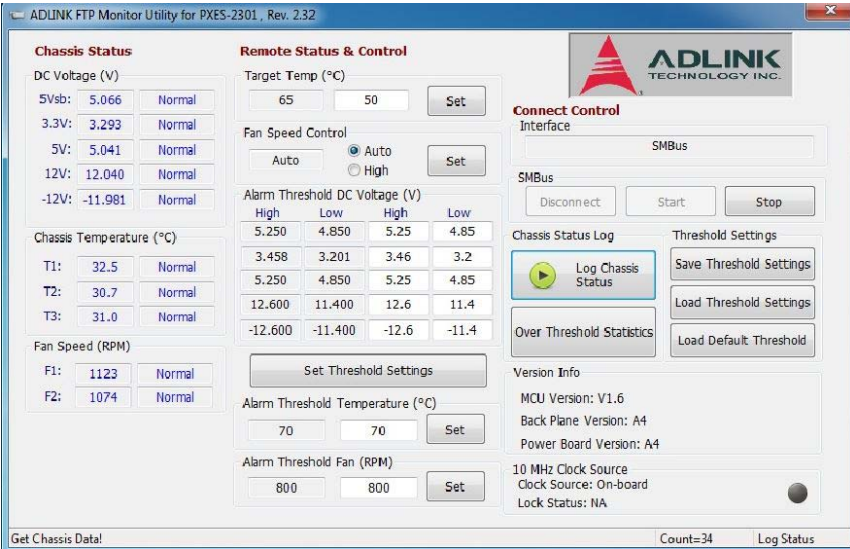


Figure 3-1: PXES-2301 Chassis Remote Mon. Utility

3.2.1 Connect Control

Selecting Connect reserves system SMBus.

Selecting Start initializes SMBus communication.

Selecting Stop ends communication.

Selecting Disconnect releases system SMBus.



NOTE:

This section is available while Interface is set to SMBus.

Chassis Status Log

With the Chassis Status Log function, monitored data can be recorded. Selecting Log Chassis Status opens the Log Options dialog, as shown.

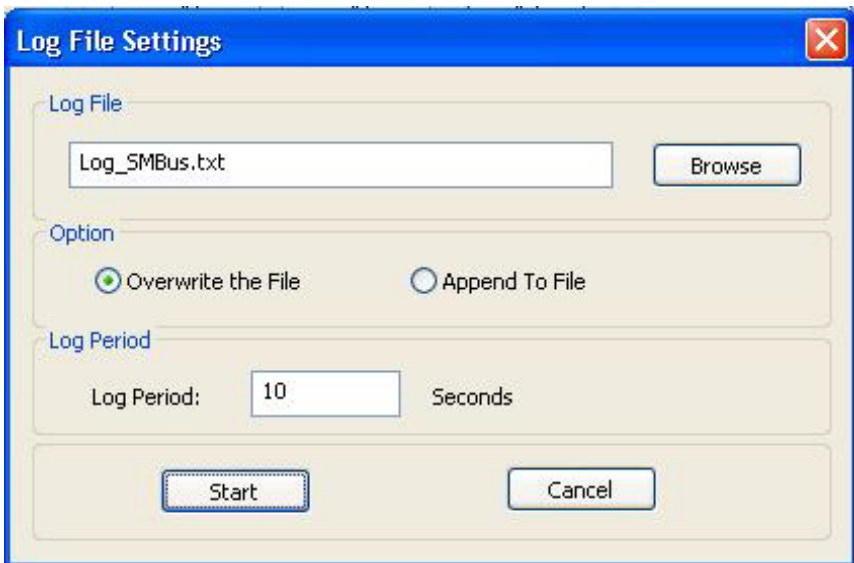


Figure 3-2: Log Options Dialog

The name of the log file can be entered, overwritten, or appended to selected operations. The log period can further be entered, in seconds. Selecting Start begins the log.

Over Threshold Statistics, when selected, displays statistics exceeding the threshold.

Save/Load Threshold

All Threshold & Control settings can be saved or loaded here.

Selecting Save Threshold Settings saves all current settings.

Selecting Load Threshold Settings loads all settings from the saved file.

Selecting Load Default Threshold resets all threshold settings to the default values XXXX f3.1.

Version Info

Displays the current firmware version.

3.2.2 Chassis Control and Alarm Threshold Setting

Provides operational and threshold settings for the PXES-2301, including trigger bus, PXIe link, target temperature, and fan mode, and threshold settings for DC voltage, temperature, and cooling fan speed.

Target Temperature

When the Fan switch on the rear panel is set to AUTO, fans run at different speeds based on the measured temperature.

Target Temp indicates the temperature at which fans run at 100%. Using the default 65°C as an example, fans run at 30% when all temperature readings are less than 25°C, and begin rampup when any reading exceeds 25°C.

Fans reach 100% speed if any temperature reading exceeds 65°C (i.e. Target Temperature).

Setting parameters are as shown.

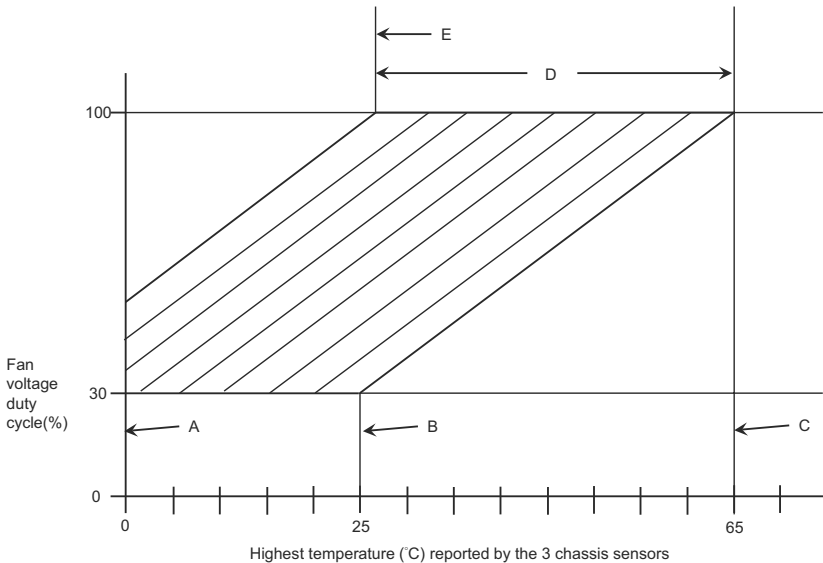


Figure 3-3: Target Temperature Parameters

Mark	Temperature	Event
A	0°C	Lowest chassis temperature at which fan speeds commence ramping up for final 25° temperature mark (see E)
B	25°C	Highest chassis temperature at which fan speeds commence ramping up for final 65° temperature mark (see C)
C	65°C	Highest chassis temperature at which fan speeds reach maximum speed
D	25°C to 65°C (40° range)	Range over which maximum chassis temperature (at which fan speeds reach maximum speed) can be set
E	25°C	Lowest chassis temperature at which fan speeds reach maximum speed

Table 3-1: Target Temperature Parameters Legend

Target Temp can be set by entering the desired target temperature value in the field and selecting Set.

Fan Speed

Displays Auto/Full fan speed setting status of the PXES-2301. Auto is displayed when fans are set to auto mode and Full when the fans are set to run at full speed.

Selection of Auto or Full values and selecting Set directly changes cooling fan mode.

Alarm Threshold

Displays Active alarm threshold settings, including DC voltage, temperature, and fan speeds. The updated threshold setting can also be set here, by entering the desired value and selecting Set Threshold Settings.

3.2.3 Chassis Status

DC Voltage

Displays monitored 5V Standby, 3.3V, 5V, 12V, and -12V power rail readings. The status displays as normal when the readings are within the threshold range, and abnormal when the threshold range is exceeded.

Chassis Temperature

Temperature sensors T1 to T3, located on the backplane provide status, display as normal when under the threshold value (70°C in the Figure), and abnormal when the threshold value is exceeded.

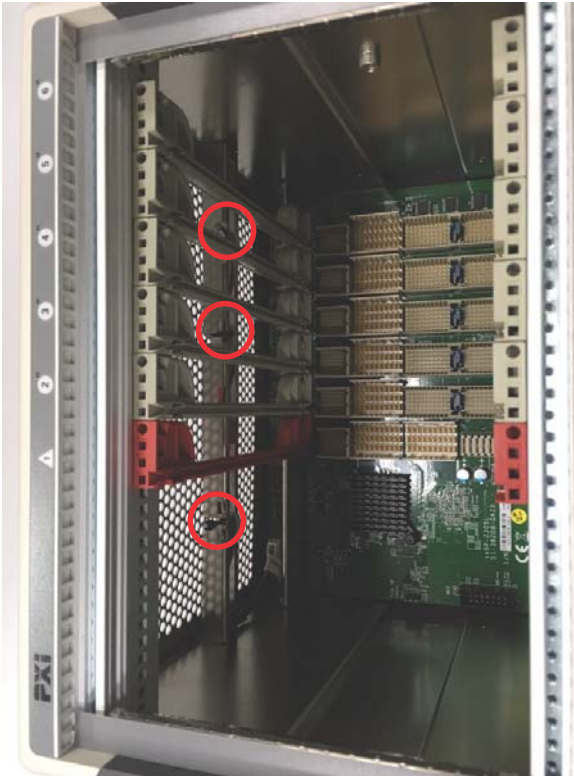


Figure 3-4: Chassis Temperature Sensors

Fan Speed

Displays monitored readings of the three cooling fans. Status displays as normal when readings exceed threshold value, and abnormal when the readings fall below the threshold value.

This page intentionally left blank.

Appendix A - Troubleshooting and Maintenance

This Appendix describes basic troubleshooting techniques, as well as instructions for the maintenance of the PXES-2301 chassis.

A.1 Installation Problems

Inability to start the system frequently results from incorrect installation of the system controller, peripheral modules, and other components. Before starting the system, please ensure that:

- ▶ The system controller is properly installed and secured
- ▶ All peripheral modules are properly seated on the slots
- ▶ All cables are properly connected to the system controller and peripheral modules
- ▶ All installed peripheral modules are compatible for use in the chassis
- ▶ The power cord is securely plugged into the chassis power connector and power outlet/wall socket/power strip

If the system fails to start when all installation conditions are met, remove all installed peripheral modules and try again. If the system starts normally, install one peripheral module at a time followed by powering up. You may also try installing the modules into different slots until the desired result is obtained.

A.2 Basic Troubleshooting

Problem	Ensure that:
System fails to power up	<ul style="list-style-type: none"> ▶ The power cord is securely plugged into the chassis power connector and wall socket/power strip ▶ The wall socket/power strip is live ▶ The power button on the chassis front panel is activated
No video output in the external display	<ul style="list-style-type: none"> ▶ The external display is functioning properly ▶ Display settings support external video.
Power LED (blue) is blinking	<ul style="list-style-type: none"> ▶ There is no short circuit by removing all PXES modules (PXES controller and peripheral modules) <p>If the signal persists, contact your dealer for further assistance</p>
Fan LED (green) is blinking	<ul style="list-style-type: none"> ▶ The fan is unobstructed <p>If the signal persists, contact your dealer for further assistance.</p>
Temperature LED (amber) is blinking	<ul style="list-style-type: none"> ▶ Airflow from the outlet apertures is unobstructed and steady; if not, ensure that adequate clearance for the intake apertures is provided <p>If the temperature of exhausted air is normal (70°C in Default setting) but the temperature LED is still blinking, contact your dealer for further assistance.</p>

A.3 Maintenance

A.3.1 Handling the Chassis

The PXES-2301 is designed for both rack-mount and benchtop use. When transporting or carrying the chassis, it is recommended

that the handle be used, being designed to support the weight of the chassis for superior portability and balance.

The PXES-2301 weighs 5.85 kg (12.9 lb). Caution should be exercised when moving the chassis to avoid any possible injury.

A.3.2 Cleaning the Exterior

Make sure that the system is turned off before cleaning the chassis exterior. Wipe the exterior with a clean cloth starting from areas that easily accumulate dust or dirt such as the area in and around the chassis and power supply air intake apertures.

A.3.3 Power Requirements


Make sure that the power cord is in good condition before plugging it into the system. It is important to check the reliability of the power source. The PXES-2301 power supply is capable of handling 100 to 240 V AC within the 50 Hz to 60 Hz range. Do not connect the PXES-2301 to an already overloaded circuit.

This page intentionally left blank.


Appendix A - Cooling Fan Replacement

The PXES-2301's easily replaced fan units significantly reduce maintenance efforts.


1. Invert the PXES-2301 chassis such that the underside is facing up.
2. Remove the four screws from the fan module cover.

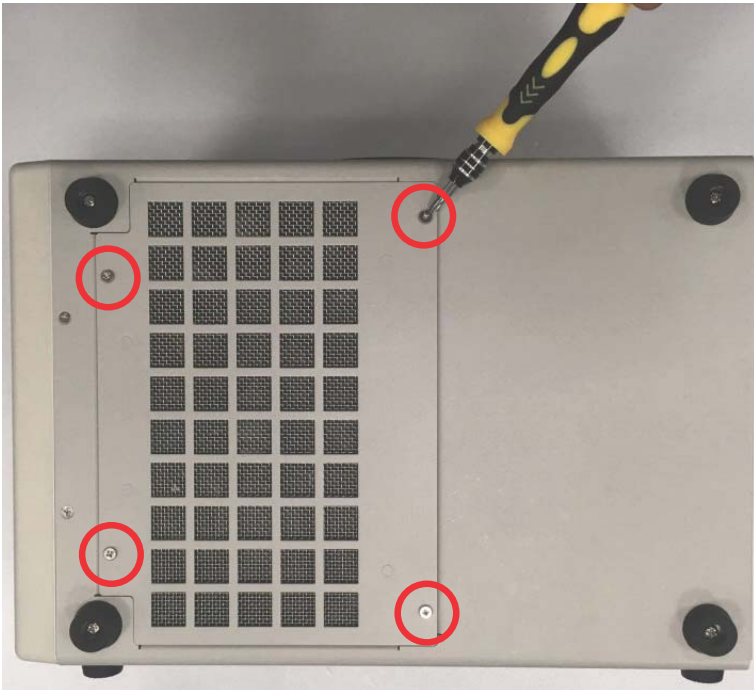


3. Remove the fan module cover and detach the two cable harnesses connected to the backplane.

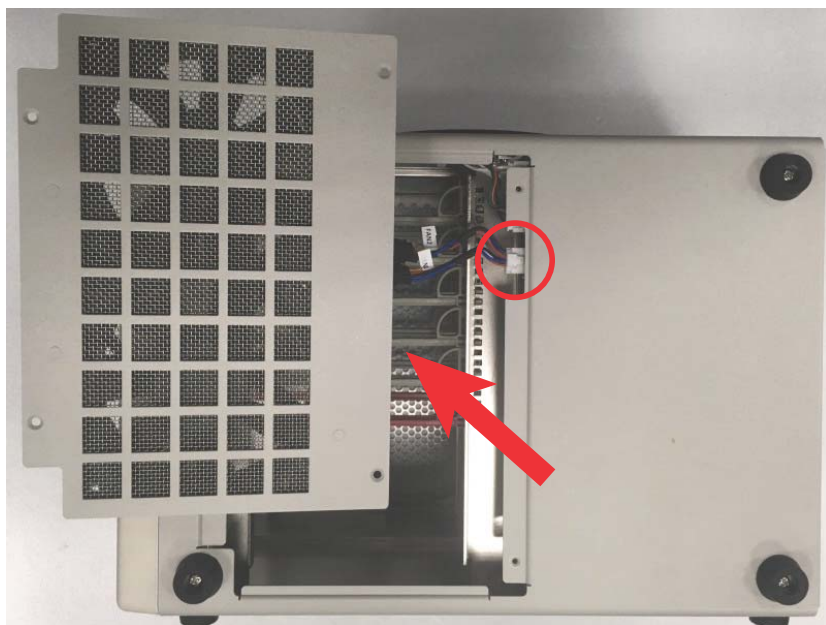

4. Withdraw the fan module from the chassis and remove the eight fixing screws.

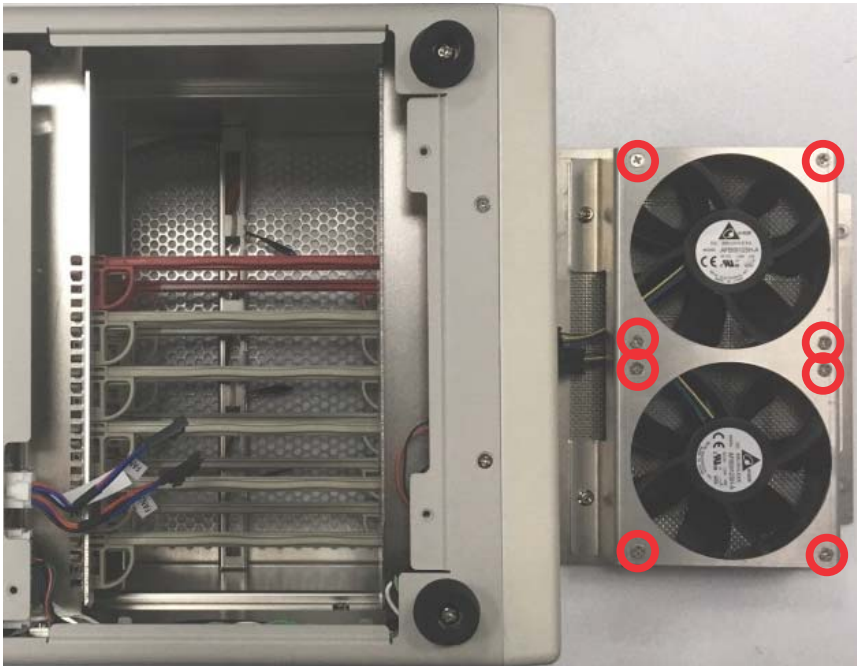

5. Remove the two cooling fan units from the module and replace with new units.

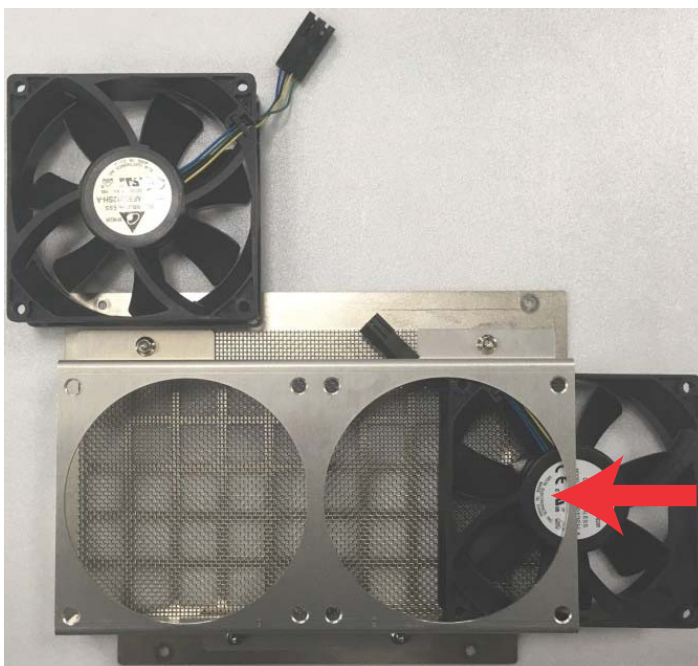

6. Replace the fixing screws and reseal the fan module in the chassis. Replace the cover.

Important Safety Instructions

For user safety, please read and follow all instructions, Warnings, Cautions, and Notes marked in this manual and on the associated device before handling/operating the device, to avoid injury or damage.

S'il vous plaît prêter attention stricte à tous les avertissements et mises en garde figurant sur l'appareil , pour éviter des blessures ou des dommages.

- ▶ Read these safety instructions carefully
- ▶ Keep the User's Manual for future reference
- ▶ Read the Specifications section of this manual for detailed information on the recommended operating environment
- ▶ The device can be operated at an ambient temperature of 50°C
- ▶ When installing/mounting or uninstalling/removing device; or when removal of a chassis cover is required for user servicing (See "Getting Started" on page 17.):
 - ▷ Turn off power and unplug any power cords/cables
 - ▷ Reinstall all chassis covers before restoring power
- ▶ To avoid electrical shock and/or damage to device:
 - ▷ Keep device away from water or liquid sources
 - ▷ Keep device away from high heat or humidity
 - ▷ Keep device properly ventilated (do not block or cover ventilation openings)
 - ▷ Always use recommended voltage and power source settings
 - ▷ Always install and operate device near an easily accessible electrical outlet
 - ▷ Secure the power cord (do not place any object on/over the power cord)
 - ▷ Only install/attach and operate device on stable surfaces and/or recommended mountings
- ▶ If the device will not be used for long periods of time, turn off and unplug from its power source


- ▶ Never attempt to repair the device, which should only be serviced by qualified technical personnel using suitable tools
- ▶ A Lithium-type battery may be provided for uninterrupted backup or emergency power.



Risk of explosion if battery is replaced with one of an incorrect type; please dispose of used batteries appropriately.

Risque d'explosion si la pile est remplacée par une autre de type incorrect. Veuillez jeter les piles usagées de façon appropriée.

- ▶ The device must be serviced by authorized technicians when:
 - ▷ The power cord or plug is damaged
 - ▷ Liquid has entered the device interior
 - ▷ The device has been exposed to high humidity and/or moisture
 - ▷ The device is not functioning or does not function according to the User's Manual
 - ▷ The device has been dropped and/or damaged and/or shows obvious signs of breakage
- ▶ Disconnect the power supply cord before loosening the thumbscrews and always fasten the thumbscrews with a screwdriver before starting the system up
- ▶ It is recommended that the device be installed only in a server room or computer room where access is:
 - ▷ Restricted to qualified service personnel or users familiar with restrictions applied to the location, reasons therefor, and any precautions required
 - ▷ Only afforded by the use of a tool or lock and key, or other means of security, and controlled by the authority responsible for the location

 A yellow triangular warning sign with a black border. Inside the triangle, there are three wavy vertical lines above a horizontal line, representing heat or a hot surface.	<p>BURN HAZARD</p> <p>Touching this surface could result in bodily injury. To reduce risk, allow the surface to cool before touching.</p> <p><i>RISQUE DE BRÛLURES</i></p> <p><i>Ne touchez pas cette surface, cela pourrait entraîner des blessures.</i></p> <p><i>Pour éviter tout danger, laissez la surface refroidir avant de la toucher.</i></p>
---	--

This page intentionally left blank.

Getting Service

Ask an Expert: <http://askanexpert.adlinktech.com>

ADLINK Technology, Inc.

Address: 9F, No.166 Jian Yi Road, Zhonghe District
New Taipei City 235, Taiwan
新北市中和區建一路 166 號 9 樓
Tel: +886-2-8226-5877
Fax: +886-2-8226-5717
Email: service@adlinktech.com

Ampro ADLINK Technology, Inc.

Address: 5215 Hellyer Avenue, #110
San Jose, CA 95138, USA
Tel: +1-408-360-0200
Toll Free: +1-800-966-5200 (USA only)
Fax: +1-408-360-0222
Email: info@adlinktech.com

ADLINK Technology (China) Co., Ltd.

Address: 上海市浦东新区张江高科技园区芳春路 300 号 (201203)
300 Fang Chun Rd., Zhangjiang Hi-Tech Park
Pudong New Area, Shanghai, 201203 China
Tel: +86-21-5132-8988
Fax: +86-21-5132-3588
Email: market@adlinktech.com

ADLINK Technology Beijing

Address: 北京市海淀区上地东路 1 号盈创动力大厦 E 座 801 室(100085)
Rm. 801, Power Creative E, No. 1 Shang Di East Rd.
Beijing, 100085 China
Tel: +86-10-5885-8666
Fax: +86-10-5885-8626
Email: market@adlinktech.com

ADLINK Technology Shenzhen

Address: 深圳市南山区科技园南区高新南七道 数字技术园
A1 栋 2 楼 C 区 (518057)
2F, C Block, Bldg. A1, Cyber-Tech Zone, Gao Xin Ave. Sec. 7
High-Tech Industrial Park S., Shenzhen, 518054 China
Tel: +86-755-2643-4858
Fax: +86-755-2664-6353
Email: market@adlinktech.com

LiPPERT ADLINK Technology GmbH

Address: Hans-Thoma-Strasse 11
D-68163 Mannheim, Germany
Tel: +49-621-43214-0
Fax: +49-621 43214-30
Email: emea@adlinktech.com

PENTA ADLINK Technology GmbH

Ulrichsbergerstrasse 17
94469 Deggendorf, Germany
Tel: +49 (0) 991 290 94 – 10
Fax: +49 (0) 991 290 94 - 29
Email: emea@adlinktech.com

ADLINK Technology, Inc. (French Liaison Office)

Address: 6 allée de Londres, Immeuble Ceylan
91940 Les Ulis, France
Tel: +33 (0) 1 60 12 35 66
Fax: +33 (0) 1 60 12 35 66
Email: france@adlinktech.com

ADLINK Technology Japan Corporation

Address: 〒101-0045 東京都千代田区神田鍛冶町 3-7-4
神田 374 ビル 4F
KANDA374 Bldg. 4F, 3-7-4 Kanda Kajicho,
Chiyoda-ku, Tokyo 101-0045, Japan
Tel: +81-3-4455-3722
Fax: +81-3-5209-6013
Email: japan@adlinktech.com

ADLINK Technology, Inc. (Korean Liaison Office)

Address: 경기도 성남시 분당구 수내로 46 번길 4 경동빌딩 2 층
(수내동 4-4 번지) (우) 463-825
2F, Kyungdong B/D, 4 Sunae-ro 46 beon-gil
Bundang-gu, Seongnam-si, Gyeonggi-do, Korea, 463-825
Toll Free +82-80-800-0585
Tel: +82-31-786-0585
Fax: +82-31-786-0583
Email: korea@adlinktech.com

ADLINK Technology Singapore Pte. Ltd.

Address: 84 Genting Lane #07-02A, Cityneon Design Centre
Singapore 349584
Tel: +65-6844-2261
Fax: +65-6844-2263
Email: singapore@adlinktech.com

ADLINK Technology Singapore Pte. Ltd. (Indian Liaison Office)

Address: #50-56, First Floor, Spearhead Towers
Margosa Main Road (between 16th/17th Cross)
Malleswaram, Bangalore - 560 055, India
Tel: +91-80-65605817, +91-80-42246107
Fax: +91-80-23464606
Email: india@adlinktech.com

ADLINK Technology, Inc. (Israeli Liaison Office)

Address: 27 Maskit St., Corex Building
PO Box 12777
Herzliya 4673300, Israel
Tel: +972-54-632-5251
Fax: +972-77-208-0230
Email: israel@adlinktech.com

ADLINK Technology, Inc. (UK Liaison Office)

Tel: +44 774 010 59 65
Email: UK@adlinktech.com